
CPM Conditioned Pain Modulation

"Expression of inhibition at the lower end of the pain scale (mechanical) is unlike the expression at the high end of the scale(thermal), which may better reflect clinical pain"

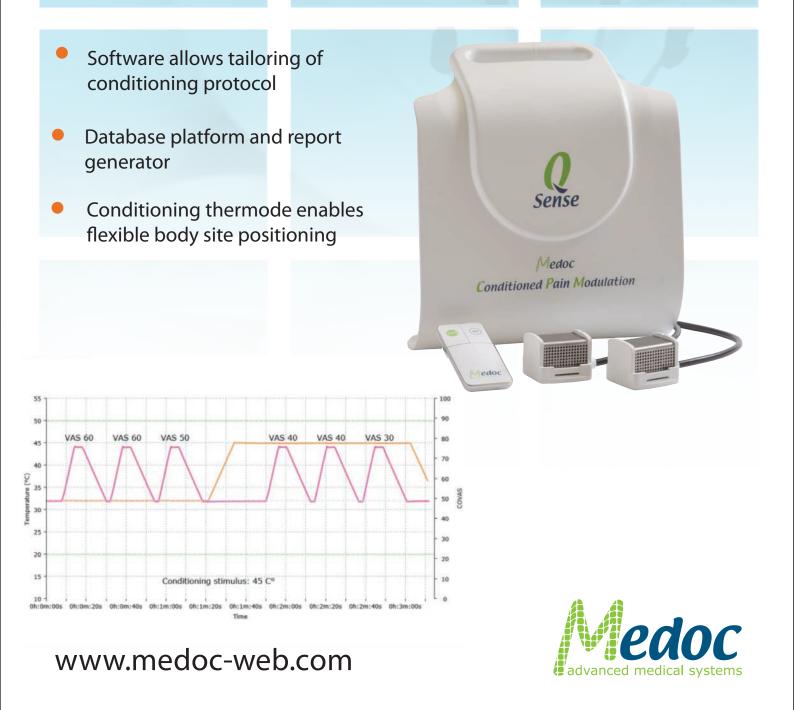

CPM Conditioned Pain Modulation

TECHNICAL SPECIFICATIONS

Thermal Sensory Analyzer, TSA-2001, Model: Q-Sense-CPM

Test Stimulation Methods	Limits Levels TSL Ramp & Hold (with optional pain rating)
Patient Response Input Devices	2 button (Yes\ No) Response Unit CoVAS (optional)
Test Results Export Options	Various formats including Excel, PDF, JPEG and etc.
Reports	Automatic reports including patient data, test information, stimulated body sites, numerical and graphical representation of test results. Comparison between results with / without conditioning stimulation
Thermode Active Area	30x30 mm
Temperature Range	20°C – 50°C
Temperature Increase Rate	0.1°C/sec – 2°C/sec
Temperature Decrease Rate	0.1°C/sec – 1°C/sec
Target Temperature Resolution	0.1°C
Display Resolution	0.1°C
Repeatability	± 0.3°C
Absolute Accuracy	± 0.3°C
Size, Weight and Form	Approx. 10 Kg, Portable Tabletop Unit
Operating Voltage	100 – 240 VAC, 4 – 2 A, 50/60 Hz
Power Consumption	Approx. 60W
Conditioning Stimulation Methods	Ramp & Hold
Test – Conditional Stimuli	Manual (via keyboard)
Synchronization	Automatic (configurable timing)







Medoc Advanced Medical Systems, USA I Compass Medical Technologies, Inc 1502 West Highway 54 - Suite 404, Durham, North Carolina 27707 phone: 919.402.9600 I Fax: 919.402.9607 I medoc@mindspring.com

Medoc Ltd. Advanced Medical Systems I World Headquarters 1 Ha'Dekel St. PO.Box 423 Ramat Yishai, Israel 30095 phone: +972-4-903.8800 I Fax: +972-4-903.8808 I medoc@medoc-web.com

EC REP EU Authorized Representative CEpartner4U BV Esdoornlaan 13 3951 DB Maan, The Netherlands, office@CEpartner4U.nl phone: +31-343-442.524 | mobile: +31-6-516-536.26 | Fax: +31-343-442.162

